

Is This Pacemaker Functioning Abnormally?

ECG CHALLENGE

An 85-year-old man with a history of ischemic heart disease and a single-chamber pacemaker implanted 6 months earlier because of atrial fibrillation with slow ventricular response was admitted to the emergency department with complaints of lightheadedness. A 12-lead ECG was obtained to assess pacemaker function as part of the initial diagnostic evaluation (Figure 1). Pacing stimuli follow an irregular pattern, as can be observed in the ECG tracing. Some pacing outputs are delivered right after the QRS complex. As a result, concerns about pacemaker malfunction arose. What is the current pacing mode in this case?

1. Normal VI function with true fusion and pseudofusion complexes, or
2. Normal VT function

Please turn the page to read the diagnosis.

Eusebio García-Izquierdo, MD
 Silvia Vilches, MD
 Victor Castro, MD

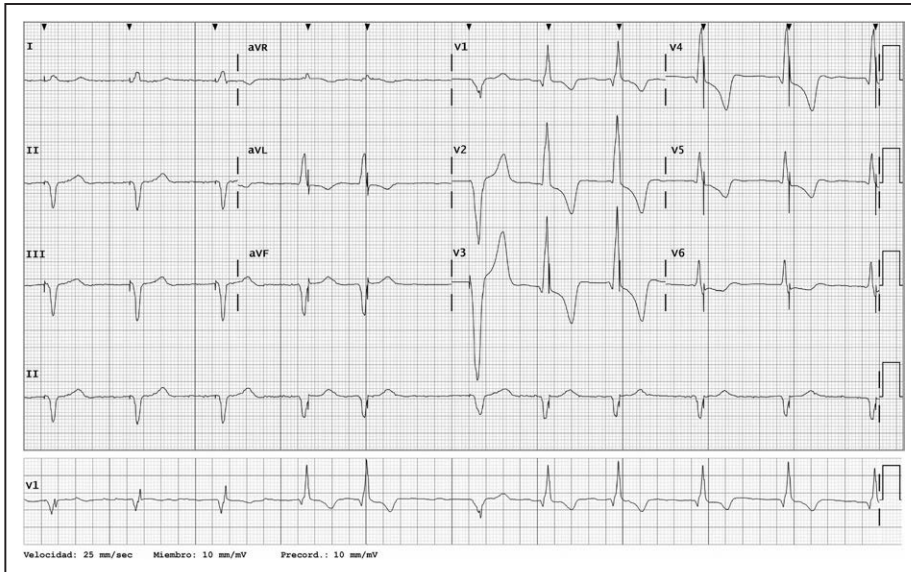


Figure 1. Twelve-lead ECG obtained at the emergency department.

Correspondence to: Eusebio García-Izquierdo, MD, Hospital Universitario Puerta de Hierro, Unidad de Arritmias, Servicio de Cardiología. Manuel de Falla, 1.28222, Majadahonda. Madrid, Spain. E-mail usegij@gmail.com

Key Words: electrical stimulation
 ■ electrocardiography
 ■ pacemaker

© 2017 American Heart Association, Inc.

RESPONSE TO ECG CHALLENGE

The rhythm is irregular without any evidence of P wave consistent with underlying atrial fibrillation. Pacing stimuli can be seen (annotated by black inverted triangles located at the top of the image in Figure 2), and QRS complexes show different morphologies according to the relationship that exists between intrinsic beats and each pacing stimulus.

QRS complexes marked with V are spontaneous beats with underlying right bundle-branch block and left anterior fascicular block. Note that the pacing stimulus falls in the last part of each QRS complex and does not follow a regular pattern, as would be expected in VVI mode.

The first 3 QRS complexes (*) are preceded by pacing stimulus at a rate of 60 bpm (\square), which is the base rate programmed in this device. The 6th QRS complex (+) is wider (0.20 second) and is also preceded by a pacing stimulus.

The differences in morphology are explained by the fact that the first 3 beats (*) are fusion beats, in which depolarization occurs partially as a result of intrinsic activation and partially as a result of capture from the pacemaker stimulus because both events are happening simultaneously, whereas the 6th-beat morphology is the result of complete pacemaker capture without fusion. Note that this 6th-beat stimulus arises at a slower heart rate (1.2 seconds=50 bpm) from the previous one

(\square); this corresponds to a lower hysteresis rate that is programmed in this case. Hysteresis is a programmable feature that allows the pacemaker to begin ventricular pacing only if the spontaneous rate falls below a set rate (in this case, 50 bpm); then pacing continues at the programmed base rate (60 bpm) unless intrinsic ventricular activity is sensed. The purpose of hysteresis is to allow a slight delay before stimulation at the base rate (ie, more time for a spontaneous QRS to occur), which preserves battery life and avoids unnecessary pacing.

The key to a correct interpretation of this ECG is given by the spontaneous QRS complexes (V). The pacing stimuli occur at the point of intrinsic QRS sensing, meaning that every spontaneous event sensed within the ventricular chamber triggers ventricular pacing. This triggered mode is called VT (pacing the ventricle, sensing the ventricle, trigger in response to sensed event). In this mode, pacing occurs at a fixed rate (in this case, 60 bpm), but in response to a sensed ventricular beat, instead of inhibiting pacing as in the VVI mode, the VVT pacemaker immediately “releases” or “triggers” a pacing stimulus. Stand-alone VT pacemakers are now obsolete, but the VT mode remains as a programmable option in many modern systems. In the past, the VT mode was used to avoid inappropriate device inhibition caused by external interference. It is important to note that this stimulus produces a “functional noncapture” because the output pulse

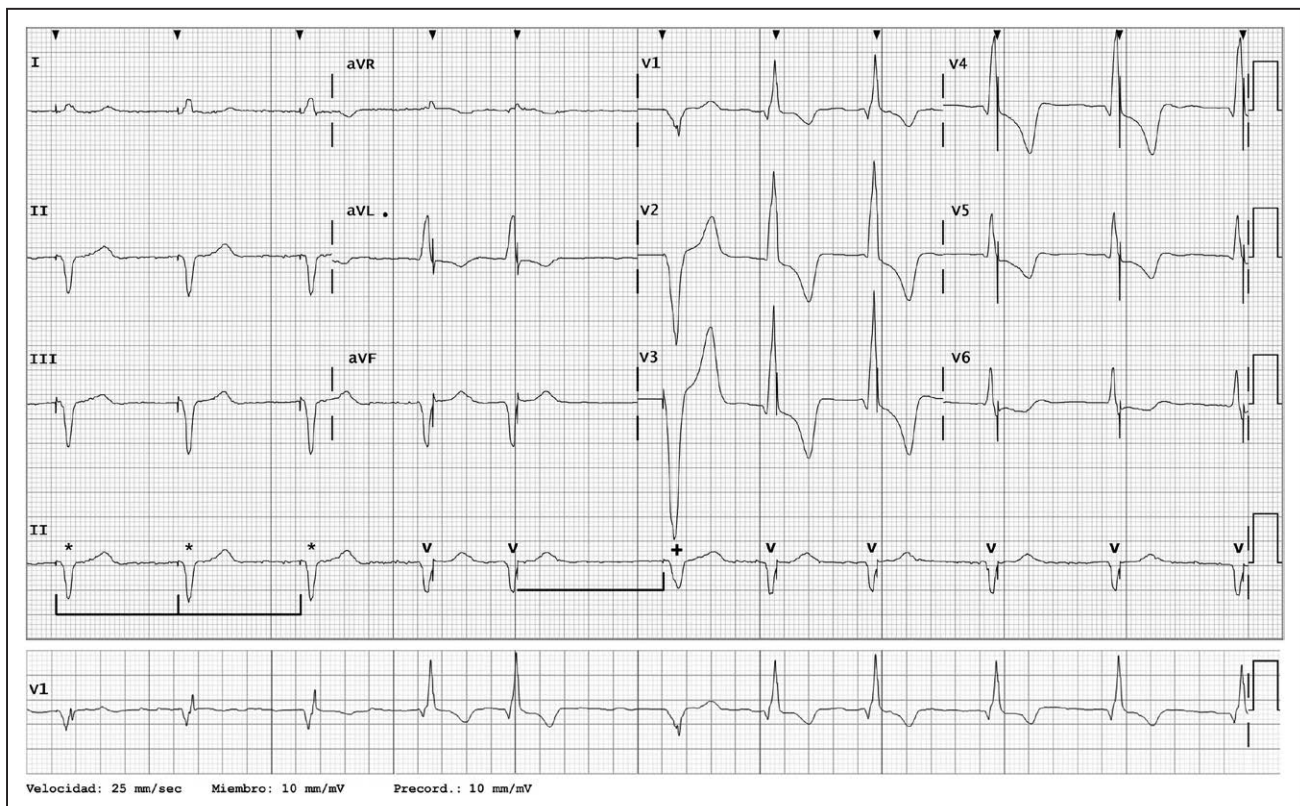


Figure 2. Twelve-lead ECG obtained at the emergency department. Annotations have been added to help interpretation.

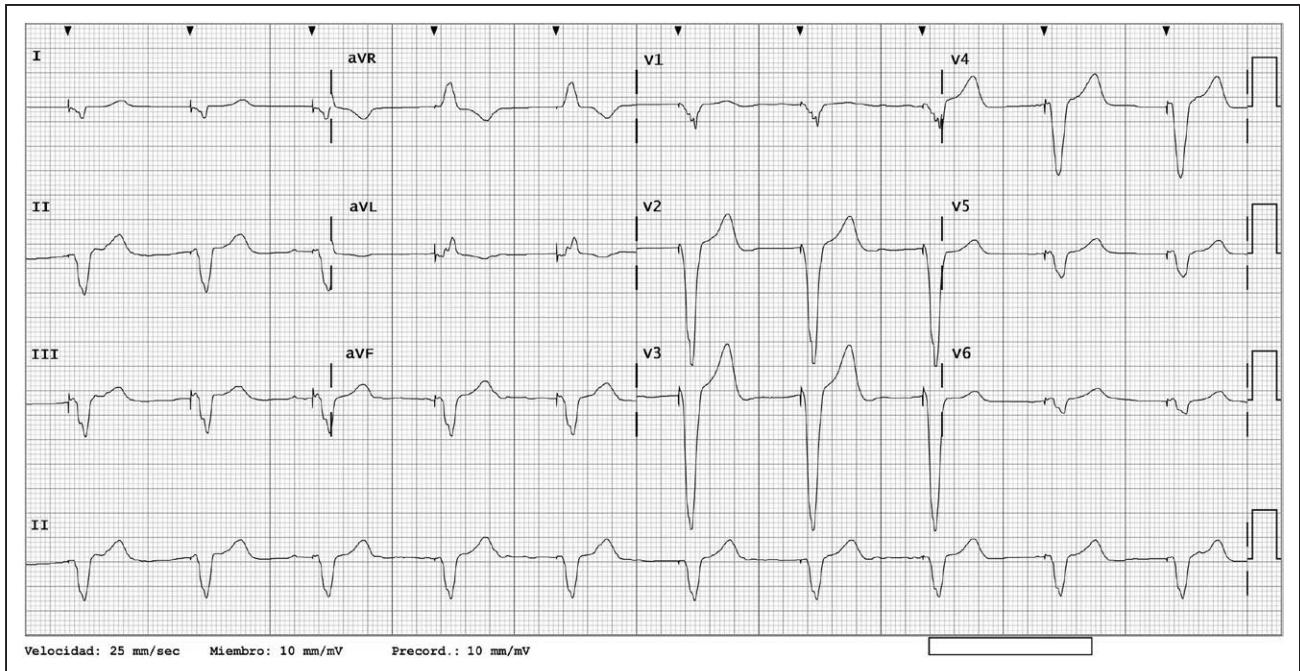


Figure 3. Twelve-lead ECG performed after changing pacing mode to VVI with a base rate of 60 bpm.

falls within the absolute refractory period of the ventricle. Similarly, pseudofusion beats may also produce “functional noncapture,” in which the pacemaker stimulus does not alter the intrinsic QRS morphology on the surface ECG. However, as opposed to the VT mode, the pacing stimulus in pseudofusion would occur at a regular programmed base rate and would fall earlier in the QRS.

This patient’s pacemaker, although mistakenly programmed in the VT mode after implantation, was functioning normally. The pacing mode was then changed to VVI to avoid excessive battery drainage, as can be seen in Figure 3.

DISCLOSURES

None.

AFFILIATIONS

From Hospital Universitario Puerta de Hierro, Majadahonda, Madrid, Spain.

FOOTNOTES

Circulation is available at <http://circ.ahajournals.org>.

Is This Pacemaker Functioning Abnormally? Eusebio García-Izquierdo, Silvia Vilches and Victor Castro

Circulation. 2017;135:711-713

doi: 10.1161/CIRCULATIONAHA.116.025972

Circulation is published by the American Heart Association, 7272 Greenville Avenue, Dallas, TX 75231

Copyright © 2017 American Heart Association, Inc. All rights reserved.

Print ISSN: 0009-7322. Online ISSN: 1524-4539

The online version of this article, along with updated information and services, is located on the
World Wide Web at:

<http://circ.ahajournals.org/content/135/7/711>

Permissions: Requests for permissions to reproduce figures, tables, or portions of articles originally published in *Circulation* can be obtained via RightsLink, a service of the Copyright Clearance Center, not the Editorial Office. Once the online version of the published article for which permission is being requested is located, click Request Permissions in the middle column of the Web page under Services. Further information about this process is available in the [Permissions and Rights Question and Answer](#) document.

Reprints: Information about reprints can be found online at:
<http://www.lww.com/reprints>

Subscriptions: Information about subscribing to *Circulation* is online at:
<http://circ.ahajournals.org/subscriptions/>